

Appendix: Long term kinetic measurements revealing precision and general performance of Surface Plasmon Resonance biosensors_Steinicke et al

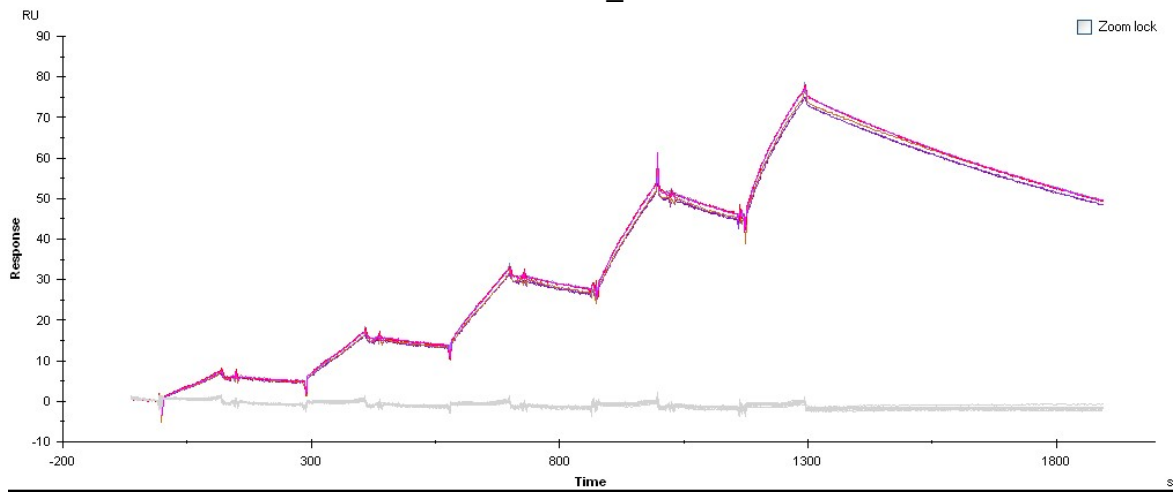


Fig A.1: Overlay of six consecutively recorded single cycle kinetics (SCK1)

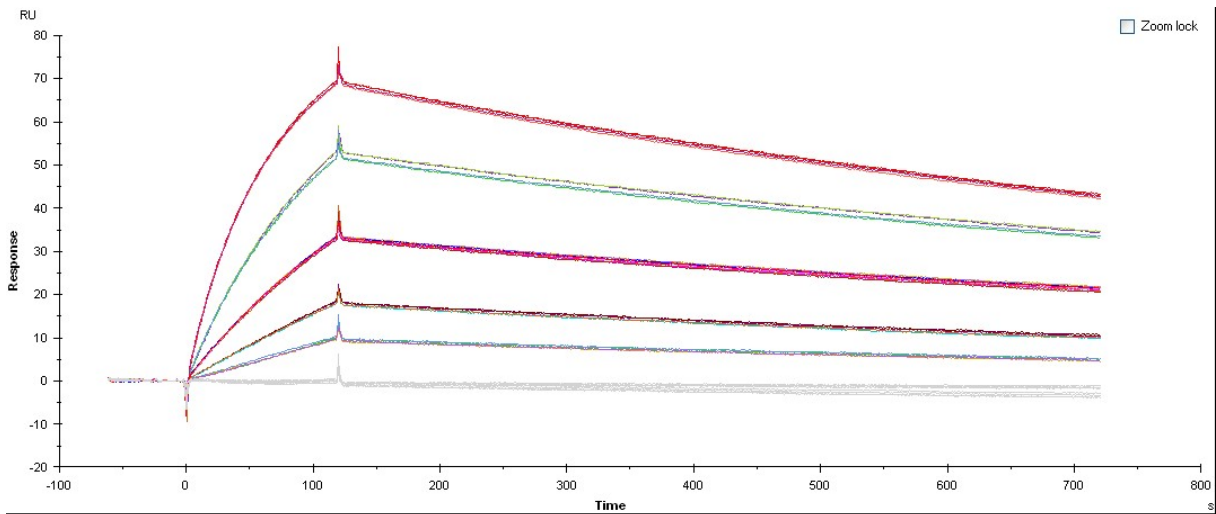


Fig A.1: Overlay from six consecutively recorded multi cycle kinetics (MCK1)

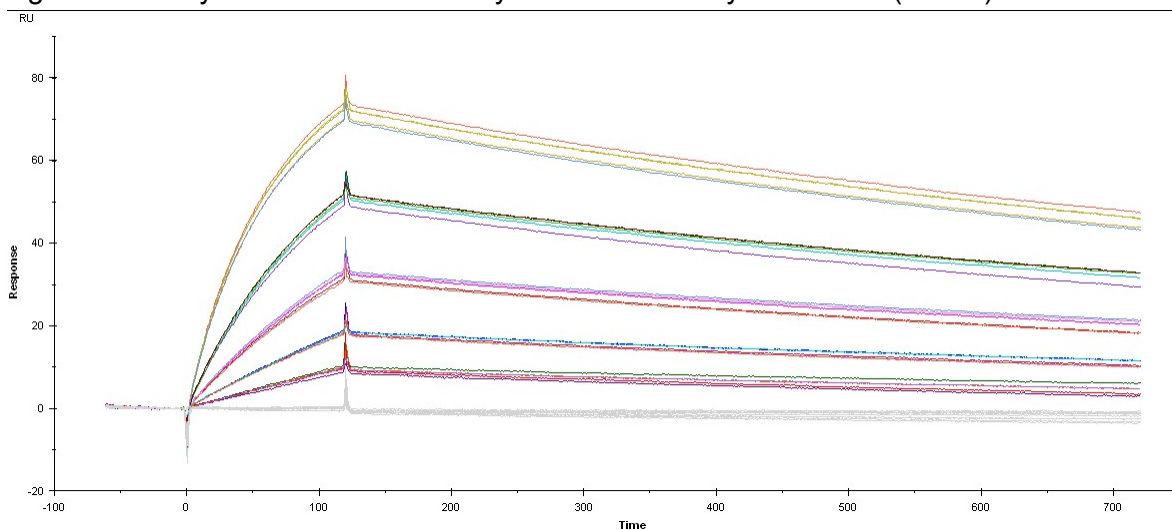


Fig A.1: Overlay of the five sample sequences almost consecutively recorded multi cycle kinetics (MCK2)